

HPLC Analysis Report

Sample: Finasteride

Buffer A: 0.04% TFA in 100% water(v/v)

Buffer B: 0.04% TFA in 100% acetonitrile (v/v)


Gradient: 10-80% Buffer B in 25 min

Flow: 1ml/min Wavelength:220nm

Column: Alltima C18,4.6*250mm,5um

Date: May. 28, 2014

Chromatogram

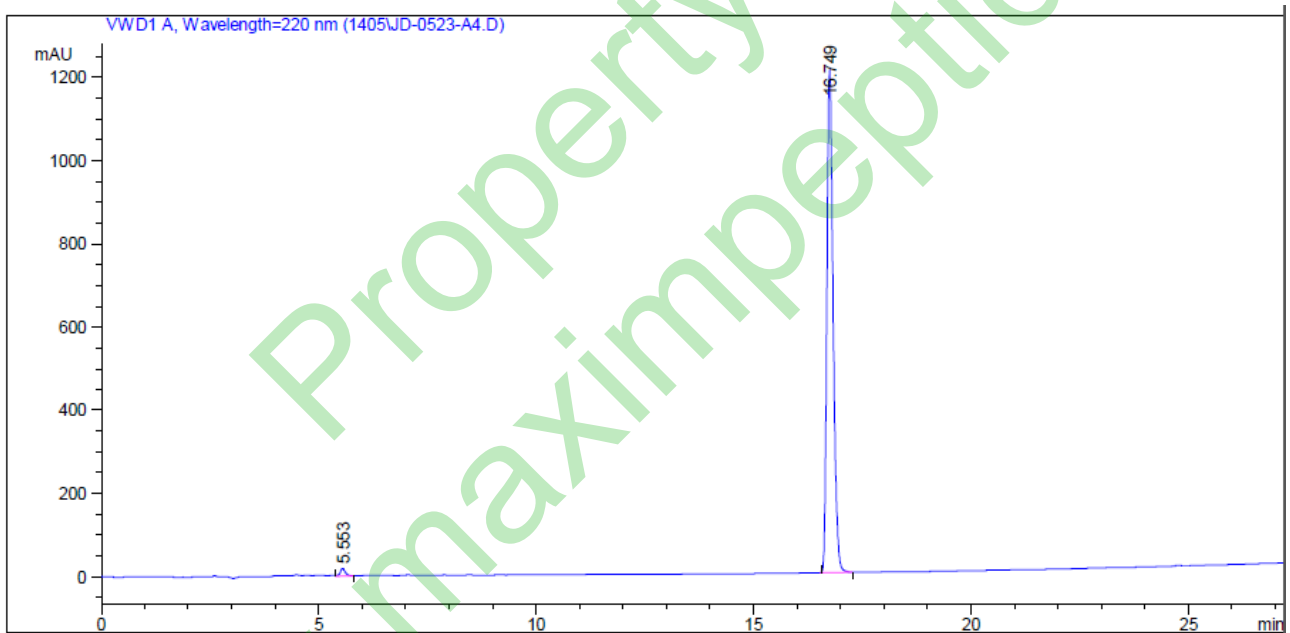

| Peak# | RetTime(Min) | Width(Min) | Area(mAU*s) | Height(mAU) | Area(%) |
|--------|--------------|------------|-------------|-------------|---------|
| 1 | 5.553 | 0.1250 | 149.11472 | 18.13680 | 1.2284 |
| 2 | 16.749 | 0.1512 | 1.19902e4 | 1203.09387 | 98.7716 |
| Totals | | | 1.21393e4 | 1221.23067 | 100 |